How to use BTNX COVID-19 Rapid antigen tests

1 SET UP

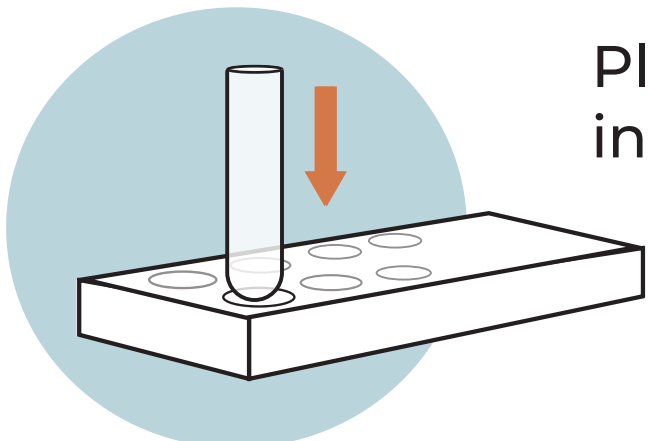

Place the tube in the holder

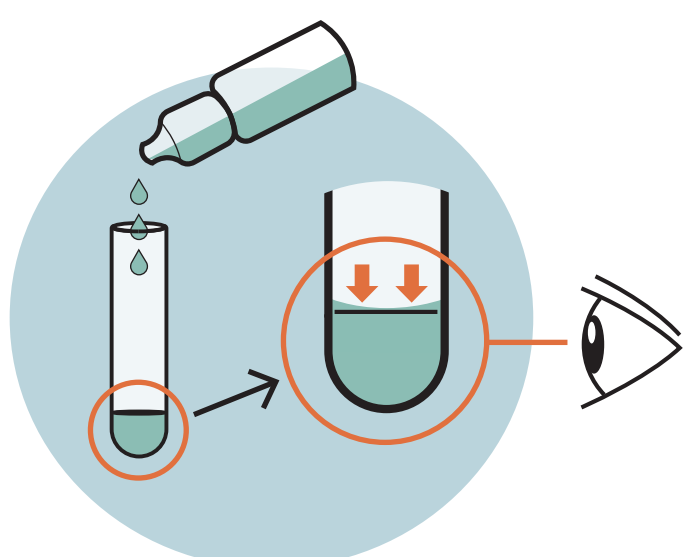

Fill the tube with the test liquid **up to the first line**

2 COLLECTION



Peel down and remove nasal swab

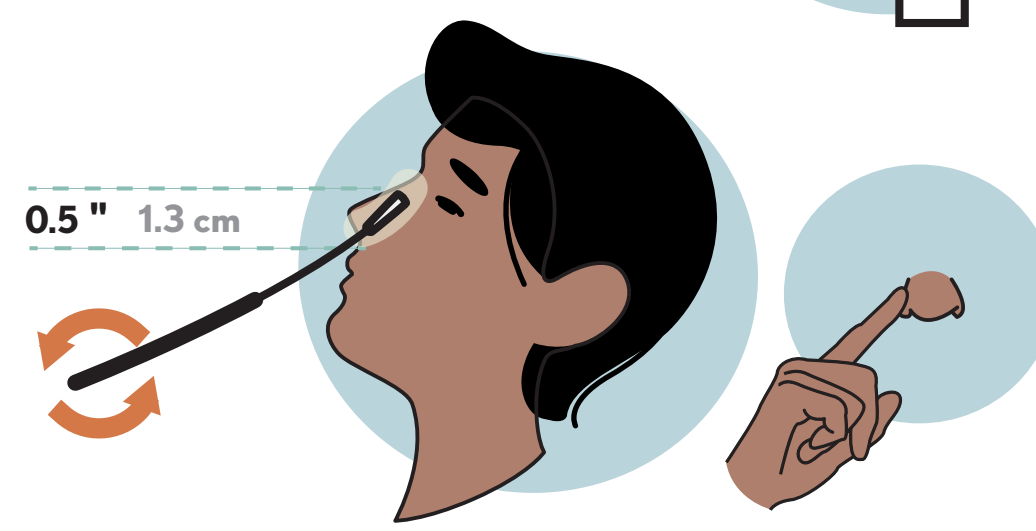

Compress the nostril with your finger as you turn the nasal swab

Insert nasal swab up to **0.5 inch (1.3 cm)** from edge of nostril. Roll **5 times** in **each nostril** (right & left)

3 PREPARATION

Insert the swab in the tube liquid and rotate it **10 times**



Place the tube and swab in the holder and leave it there for **2 minutes**

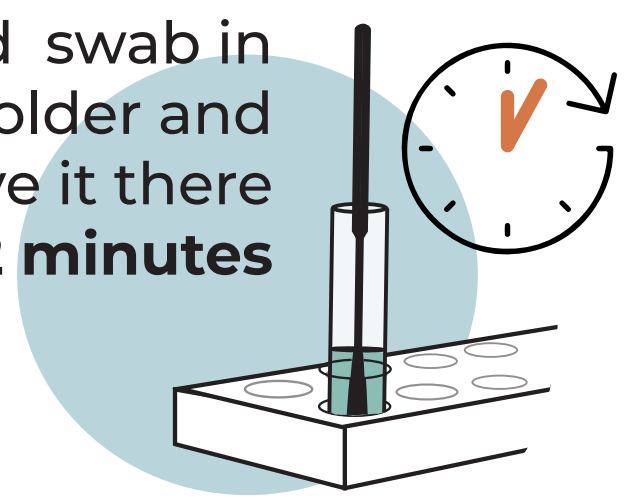

Remove the swab by pinching the tube



Close the tube with the stopper cap



4 TESTING

Place **3 drops** in the rapid response cartridge and **wait 15 minutes**

(Do not touch it during the waiting time)

Here is an example of a positive test, negative and an invalid test

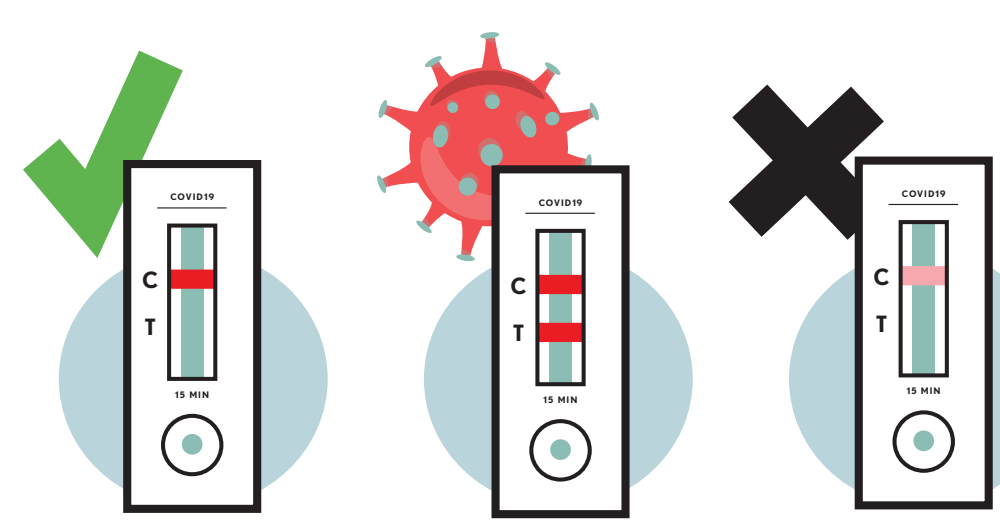

NEGATIVE **POSITIVE** **INVALID**

Redo the nasal swab with a new kit.

Please call the COVID-19 Infoline: **1-866-855-2811**

ᒥᔪᐲᒫᑎᓰᐅᓐ ᐊᓈᓈᑭᒋᐦᑖᑲᓅᒡ
CONSEIL CRI DE LA SANTÉ ET DES SERVICES SOCIAUX DE LA BAIE JAMES
CREE BOARD OF HEALTH AND SOCIAL SERVICES OF JAMES BAY

(Graphics adapted from Nunavik Regional Board of Health and Social Services - NRBHSS)

For more information:
CREEHEALTH.ORG/COVID